

Digital Pressure Gauge / Pressure Switch

Application

- Hygienic pressure measurement
- Overpressure save at highest accuracy
- Largest display in a process gauge

Application examples

- Local display without external power supply
- Pressure switch with two relays

Hygienic design / Process connection

- Hygienic process connection with CLEANadapt
- Conforming to 3-A Sanitary Standard for versions with DIRECTadapt
- All wetted materials are FDA-conform
- All materials and actuating fill are FDA conform
- complete overview of process connections: see order code
- The Anderson-Negele CLEANadapt system offers a flow-optimized, hygienic and easily sterilizable installation solution for sensors.

Features

- CIP-/ SIP-cleaning up to 149 °C / 60 minutes maximum
- IP 66, housing for optimized cleanability
- 2-fold overpressure safety as standard
- Protected calibration possibility
- Standard min. / max. pressure caption feature
- Display height 23 mm
- Charge level indicator for battery
- Display units: BAR, PSI, H₂O, mmHg, inHg, MPa, kPa

Options

- Two independent relays with external power supply
- MAN-90P-BAT: phar maversion with $R_a \leq 0.2 \mu\text{m}$ wetted part
- Hastelloy membrane wetted parts

Authorizations



MAN-90x-BAT / S / ...




MAN-90-BAT		
Material	diaphragm fitting case inspection window	316L, optional: Hastelloy C 1.4404 1.4301, complete welded polysulfone (for temperatures up to 163 °C)
Surface roughness	diaphragm	$R_a \leq 0.6 \mu\text{m}$ standard
Actuating fill		paraffin oil / medical white oil FDA approval number 21 CFR 172.828 and 178.3620 (a)
Protection Class		IP 66 / NEMAX 4X
Overpressure safety		2-fold
Accuracy		0.2 % of full scale
Repeatability		± 0.06 % of full scale
Linearity		± 0.07 % of full scale
Hysteresis		± 0.07 % of full scale
Temperature	process CIP- / SIP-cleaning ambient	-4 °C...130 °C 149 °C / 60 minutes maximum 4 °C...50 °C
Temperature effect		$< \pm 0.16$ % / 10 K of full scale (process or ambient)
Display	LED height dampening	23 mm programmable additional display of battery status and alarm 1 and 2 indicators
Power Supply	for LCD for relay	batteries 2 x AA 9...30 V DC, 250 mA battery back up of programmed values
Output	2x switch (relay) (open with no power) function and hysteresis	24 V DC, max. 1 A programmable
Approvals / Standards	PED EMV-conformity	3-A PED-SEP IEC 61326
Weight	fitting CLEANadapt G1" Tri-Clamp 1,5" Tri-Clamp 2" mounting position back	830 g 690 g 710 g additional 50 g

MAN-90P-BAT (Pharma version)


Surface roughness $R_a \leq 0.2 \mu\text{m}$

Conform to ASME BPE
Certificates provided with product


MAN-90x-BAT / S / ...

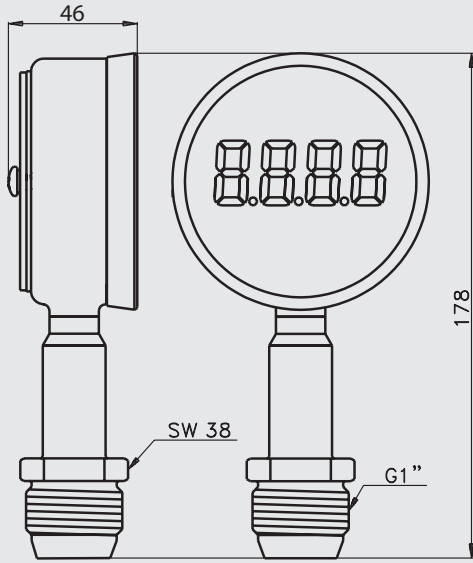

MAN-90x-BAT / TC / ... with connection U, L, R

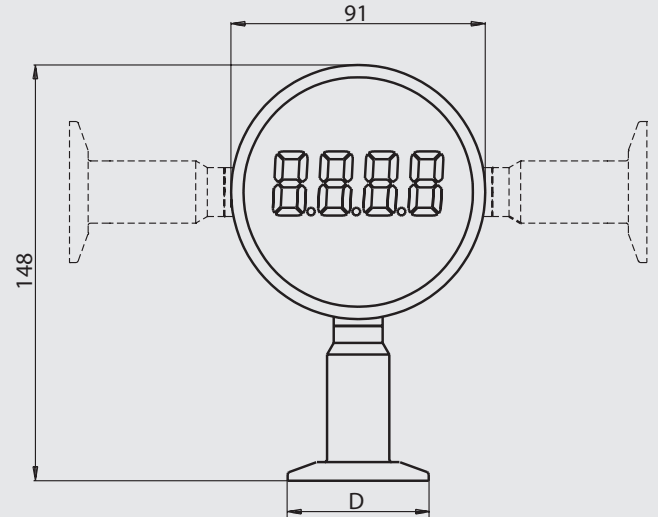


MAN-90x-BAT / TC / ... with connection H

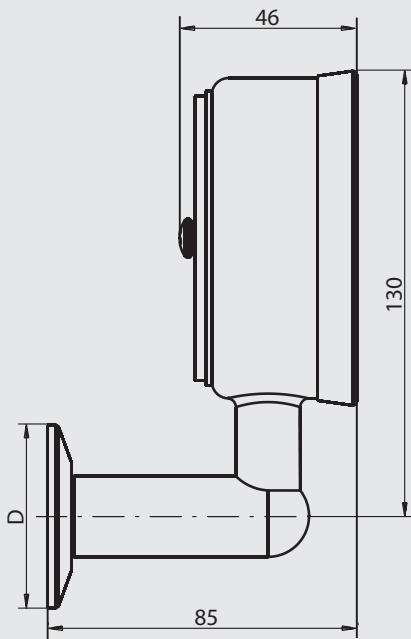


Electrical connection with M12-plug

Configuration M12-plug



- 1: + supply
- 2: - supply
- 3: relay 1 and 2 COM
- 4: relay 1 closing contact
- 5: relay 2 closing contact

Internal switches relay 1 and 2

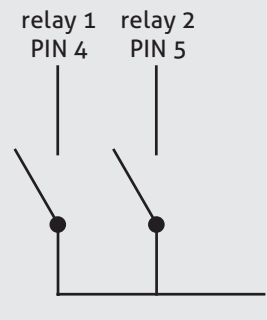

Note:
Contact voltage per relay
max 24 V DC

Dimension table Tri-Clamp

Clamp size D [mm]	Suitable for pipe diameter	Pipe style
50.5	DN 40 1½"	DIN 11866 series A DIN 11866 series B / ISO 1127 DIN 11866 series C / OD-Tube
64.0	DN 50 2"	DIN 11866 series A DIN 11866 series C / OD-Tube
77.5	2½"	DIN 11866 series C / OD-Tube
91.0	DN 65 3"	DIN 11866 series A DIN 11866 series C / OD-Tube

Conditions for a measuring point according to 3-A Sanitary Standard 74-06




- The sensors MAN-90-BAT / TC... and MAN-90P-BAT / TC... conforming to the 3-A Sanitary Standard.
- The sensors are designed for CIP-/ SIP-cleaning. Maximum 149 °C / 60 minutes.
- Only with 3-A conforming Tri-Clamp process connection..
- Mounting position, self draining and the position of the leakage hole must be in accordance to current 3-A Sanitary Standard.

Display MAN-90x-BAT

- 1. Primary display**
Four digit LCD with adjustable decimal point position to indicate pressure value.
- 2. Display setpoint 1 and 2**
Flashes if setpoint is tripped. Displays continuously during setpoint viewing or programming.
- 3. Secondary display**
Indicates pressure unit or parameter information.
- 4. Battery status display**
Three bars indicate an intact and fully charged battery.


Fig. 1: Display MAN-90x-BAT

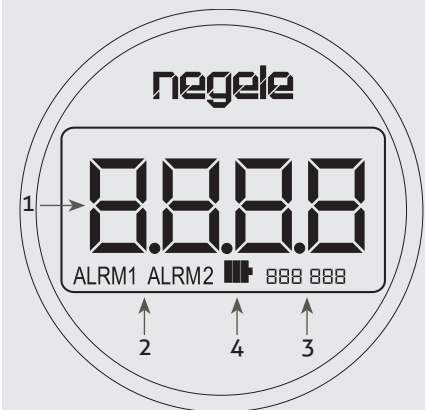

Programming MAN-90x-BAT

- To access the switches remove the two screws and the cover with gasket.
- All parameter values can be read in RUN-Mode by pressing SCROLL FWD and SCROLL BACK. After 3 sec. the gauge automatically switches to the display mode.
- MAN-90-BAT is to be programmed with the switches VALUE, RUN and MENU. Therefore you put the RUN-switch to SETPOINTS or CALIBRATION.
- To switch back to measuring mode put RUN-switch back to RUN!



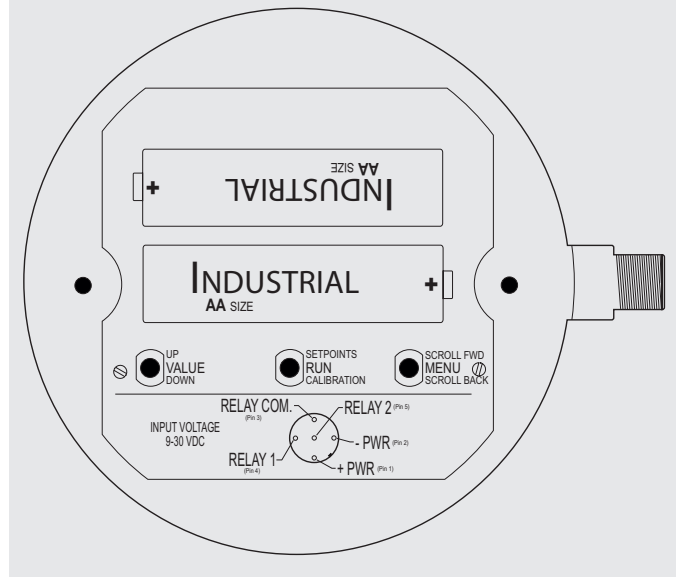







Fig. 2: MAN-90x-BAT with open lid























Attention:



While the cover is removed, do not allow moisture to enter the gauge housing.

Alarm setpoint programming (RUN-switch set to SETPOINTS)					
Value	LC-Display	Switch	Adjustment		
Alarm 1 setpoint		VALUE UP / DOWN	0...100 % of range (in pressure units) pressure at which relay 1 closes		
	↕	MENU SCROLL FWD / SCROLL BACK			
Alarm 1 action		VALUE UP / DOWN			
			Relay 1 closed above setpoint		Relay 1 closed below setpoint
	↕	MENU SCROLL FWD / SCROLL BACK			
Alarm 1 hysteresis		VALUE UP / DOWN	Alarm 1 hysteresis 0...100 % of range (in pressure units)		
	↕	MENU SCROLL FWD / SCROLL BACK			
Alarm 2 setpoint		VALUE UP / DOWN	0...100 % of range (in pressure units) pressure at which relay 2 closes		
	↕	MENU SCROLL FWD / SCROLL BACK			
Alarm 2 action		VALUE UP / DOWN			
			Relay 2 closed above setpoint		Relay 2 closed below setpoint
	↕	MENU SCROLL FWD / SCROLL BACK			
Alarm 2 hysteresis		VALUE UP / DOWN	Alarm 2 hysteresis 0...100 % of range (in pressure units)		

Calibration / Configuration programming (RUN-switch set to CALIBRATION)				
Value	LC-Display	Switch	Adjustment	
Calibration menu				
		MENU SCROLL FWD / SCROLL BACK		
Offset		VALUE UP / DOWN	Offset calibration adjustment Adds to reading Range: ± 10 % of span	
		MENU SCROLL FWD / SCROLL BACK		
Span		VALUE UP / DOWN	Span calibration adjustment Multiplies reading Range: 0.90...1.10	
		MENU SCROLL FWD / SCROLL BACK		
Displayed units		VALUE UP / DOWN	Units PSI Gau, PSI ABS, in H ₂ O, kg/cm ² , mmHg, inHg, MPa, kPa, Bar	
		MENU SCROLL FWD / SCROLL BACK		
Dampening factor		VALUE UP / DOWN	Dampening Factor Digital Filter setable from 0.0...10.0 (no dampening = 0.0)	
		MENU SCROLL FWD / SCROLL BACK		
Decimal position		VALUE UP / DOWN	Decimal point position (Setting is not stored in nonvolatile memory)	
		MENU SCROLL FWD / SCROLL BACK		
Maximum pressure captured		VALUE UP / DOWN	Hold UP-switch for 3 seconds to reset	
		MENU SCROLL FWD / SCROLL BACK		
Minimum pressure captured		VALUE UP / DOWN	Hold UP-switch for 3 seconds to reset	
		MENU SCROLL FWD / SCROLL BACK		
Restore factory defaults		VALUE UP / DOWN	Hold UP-switch for 3 seconds to reset all factory defaults	

Mechanical Connection / Installation

- Use only Negele CLEANadapt system for safe operation of measuring point!

Transport / Storage

- No outdoor storage
- Dry and dust free
- Not exposed to corrosive media
- Protected against solar radiation
- Avoiding mechanical shock and vibration
- Storage temperature -55...+90 °C
- Relative humidity maximum 98 %

Cleaning / Maintenance

- In case of using pressure washers, don't point nozzle directly to electrical connections!

Reshipment

- Sensors shall be clean and free of media or heat-conductive paste and must not be contaminated with dangerous media!
- Use suitable transport packaging only to avoid damage of the equipment!

Conventional Usage

- Not suitable for applications in explosive areas.
- Not suitable for applications in security-relevant equipments (SIL).

Standards and Guidelines

- You have to comply with applicable regulations and directives.

Note on CE

- Applicable directives: Electromagnetic Compatibility Directive 2014/30/EU
- Compliance with the applicable EU directives is identified by the CE label on the product.
- The operating company is responsible for complying with the guidelines applicable to the entire installation.

Disposal

- Electrical devices should not be disposed of with household trash. They must be recycled in accordance with national laws and regulations.
- Take the device directly to a specialized recycling company and do not use municipal collection points.

Accessories**M12-K / 5**

M12-connection 4-pin, IDC technique, with plastic knurled screw

PVC-cable with M12-connection made of 1.4305, IP 69 K, unshielded

M12-PVC / 5-5 m

PVC-cable 5-pin, length 5 m

M12-PVC / 5-10 m

PVC-cable 5-pin, length 10 m

M12-PVC / 5-25 m

PVC-cable 5-pin, length 25 m

PVC-cable with M12-connection, brass nickel-plated, IP 67, shielded

M12-PVC / 5G-5 m

PVC-cable 5-pin, length 5 m

M12-PVC / 5G-10 m

PVC-cable 5-pin, length 10 m

M12-PVC / 5G-25 m

PVC-cable 5-pin, length 25 m

M12-EVK

M12 plug-in screw cap, 1.4305 (303), with o-ring, as a protection against humidity and dirt

CAL/MAN

factory calibration certificate, incl. inspection certificate 3.1 acc. to EN 10204 (only product contacting surface)

PVC-cable with M12-connection**M12 plug-in screw cap**

Order Code

MAN-90-BAT
MAN-90P-BAT

(Food version, diameter housing 90 mm)

(Pharma version, diameter housing 90 mm, including material certificate and calibration certificate)

Process Connection with 3-A TPV approval

TC1 (Tri-Clamp 1.5")

TC2 (Tri-Clamp 2")

TC2.5 (Tri-Clamp 2.5")

TC3 (Tri-Clamp 3")

Following Process Connections only for MAN-90-BAT available (not with 3-A TPV approval)

S (CLEANadapt G1", process connection conforming to EHEDG)

Measuring Range

-1...0 (-1.0...0 bar)

-1...+1 (-1.0...+1.0 bar)

-1...+2 (-1.0...+2.0 bar)

-1...+4 (-1.0...+4.0 bar)

-1...+7 (-1.0...7.0 bar)

0...1 (0...1.0 bar)

0...2 (0...2.0 bar)

0...4 (0...4.0 bar)

0...6 (0...6.0 bar)

0...7 (0...7.0 bar)

0...10 (0...10.0 bar)

0...14 (0...14.0 bar)

0...20 (0...20.0 bar)

Connection

U (bottom)

L (left)

R (right)

H (back)

Membrane

316L (Standard)

HAST (Hastelloy C)

Switching

X (without)

1 (with 2 normally open relay contacts, 1 A max.)

MAN-90-BAT /

TC1 /

-1...+2 /

U /

316L /

X